



PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : A61B 17/00	A2	(11) International Publication Number: WO 00/18302 (43) International Publication Date: 6 April 2000 (06.04.00)
<p>(21) International Application Number: PCT/US99/22553</p> <p>(22) International Filing Date: 30 September 1999 (30.09.99)</p> <p>(30) Priority Data: 09/163,884 30 September 1998 (30.09.98) US</p> <p>(71) Applicant: C. R. BARD, INC. [US/US]; 730 Central Avenue, Murray Hill, NJ 07974 (US).</p> <p>(72) Inventors: GAMBALE, Richard, A.; 382 Dunstable Road, Tyngsboro, MA 01879 (US). AHERN, John, E.; 30 Lynn Fells Parkway, Melrose, MA 02176 (US). PARASCAN-DOLA, Michael; 14 Hazelnut Lane, Londonderry, NH 03053 (US).</p> <p>(74) Agent: PERULLO, John, F.; Kirkpatrick & Lockhart LLP, 75 State Street, Boston, MA 02109-1808 (US).</p>	<p>(81) Designated States: CA, JP, MX, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</p> <p>Published <i>Without international search report and to be republished upon receipt of that report.</i></p>	
<p>(54) Title: IMPLANT DELIVERY SYSTEM</p> <p>(57) Abstract</p> <p>The present invention provides an implant delivery system for placing interior defining implants in the human body. The devices comprise elongate shafts and a mechanism at the distal end of the shaft for engaging and retaining the implant in place on the shaft during delivery through the vessels and insertion of the distal end of the shaft into tissue. Some embodiments of the devices are configured to have a plurality of implants and configured to deliver the implants sequentially to a plurality of locations. One embodiment employs a flexible outer tube at its distal end that compresses and crinkles to a larger diameter upon being compressed lengthwise to engage the inside surface of the implant. Another embodiment utilizes a tubular delivery shaft having a circular cross section with segments of oval shaped cross sections which serve to engage the inside of implant located on the shaft. A cam slidable within the shaft engages the oval areas, deforming them to a circular shape which permits the implants to be released. Another embodiment provides delivery force by pressurizing fluid filling the shaft lumen to move a plunger at the distal end of the shaft which carries the implant to be delivered. A feature of the invention provides for monitoring of the depth to which an implant is delivered within tissue by monitoring pressure changes experienced near the distal tip of the shaft. Another feature of the delivery devices provides for drug delivery at the implant site by compressing a drug filled bladder by the expansion of an adjoining bladder. Also disclosed is the use of an electromagnetic guidance system to accurately navigate the delivery devices to the implant delivery sites.</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakhstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

IMPLANT DELIVERY SYSTEM

Field of the Invention

This invention relates to delivery devices for implants placeable within tissue of
5 the human body. Specifically, the invention relates to delivery of implants configured
to aid in the restoration of blood flow to myocardial tissue of the heart. The invention
includes a mechanism to monitor the position of the device and deliver drugs.

Background of the Invention

10 Tissue becomes ischemic when it is deprived of adequate blood flow.
Ischemia causes pain in the area of the affected tissue and, in the case of muscle
tissue, can interrupt muscular function. Left untreated, ischemic tissue can become
infarcted and permanently non-functioning. Ischemia can be caused by a blockage in
the vascular system that prohibits oxygenated blood from reaching the affected tissue
15 area. However, ischemic tissue can be revived to function normally despite the
deprivation of oxygenated blood because ischemic tissue can remain in a hibernating
state, preserving its viability for some time. Restoring blood flow to the ischemic
region serves to revive the ischemic tissue.

Although ischemia can occur in various regions of the body, often tissue of the
20 heart, the myocardium, is affected by ischemia due to coronary artery disease,
occlusion of the coronary artery, which otherwise provides blood to the myocardium.
Muscle tissue affected by ischemia can cause pain to the individual affected.
Ischemia can be treated, if a tissue has remained viable despite the deprivation of
oxygenated blood, by restoring blood flow to the affected tissue.

25 Treatment of myocardial ischemia has been addressed by several techniques
designed to restore blood supply to the affected region. Coronary artery bypass
grafting CABG involves grafting a venous segment between the aorta and the
coronary artery to bypass the occluded portion of the artery. Once blood flow is

- 2 -

redirected to the portion of the coronary artery beyond the occlusion, the supply of oxygenated blood is restored to the area of ischemic tissue.

Early researchers, more than thirty years ago, reported promising results for revascularizing the myocardium by piercing the muscle to create multiple channels for blood flow. Sen, P.K. et al., "Transmyocardial Acupuncture - A New Approach to Myocardial Revascularization", *Journal of Thoracic and Cardiovascular Surgery*, Vol. 50, No. 2, August 1965, pp. 181-189. Although others have reported varying degrees of success with various methods of piercing the myocardium to restore blood flow to the muscle, many have faced common problems such as closure of the created channels. Various techniques of perforating the muscle tissue to avoid closure have been reported by researchers. These techniques include piercing with a solid sharp tip wire, hypodermic tube and physically stretching the channel after its formation. Reportedly, many of these methods still produced trauma and tearing of the tissue that ultimately led to closure of the channel.

An alternative method of creating channels that potentially avoids the problem of closure involves the use of laser technology. Researchers have reported success in maintaining patent channels in the myocardium by forming the channels with the heat energy of a laser. Mirhoseini, M. et al., "Revascularization of the Heart by Laser", *Journal of Microsurgery*, Vol. 2, No. 4, June 1981, pp. 253-260. The laser was said to form channels in the tissue were clean and made without tearing and trauma, suggesting that scarring does not occur and the channels are less likely to experience the closure that results from healing. U.S. Patent No. 5,769,843 (Abela et al.) discloses creating laser-made TMR channels utilizing a catheter based system. Abela also discloses a magnetic navigation system to guide the catheter to the desired position within the heart. Aita patents 5,380,316 and 5,389,096 disclose another approach to a catheter based system for TMR.

Although there has been some published recognition of the desirability of performing transmyocardial revascularization (TMR) in a non-laser catheterization procedure, there does not appear to be evidence that such procedures have been put into practice. For example, U.S. Patent No. 5,429,144 Wilk discloses inserting an

- 3 -

expandable implant within a preformed channel created within the myocardium for the purposes of creating blood flow into the tissue from the left ventricle.

Performing TMR by placing stents in the myocardium is also disclosed in U.S. Patent No. 5,810,836 (Hussein et al.). The Hussein patent discloses several stent
5 embodiments that are delivered through the epicardium of the heart, into the myocardium and positioned to be open to the left ventricle. The stents are intended to maintain an open channel in the myocardium through which blood enters from the ventricle and perfuses into the myocardium.

Angiogenesis, the growth of new blood vessels in tissue, has been the subject
10 of increased study in recent years. Such blood vessel growth to provide new supplies of oxygenated blood to a region of tissue has the potential to remedy a variety of tissue and muscular ailments, particularly ischemia. Primarily, study has focused on perfecting angiogenic factors such as human growth factors produced from genetic engineering techniques. It has been reported that injection of such a growth factor
15 into myocardial tissue initiates angiogenesis at that site, which is exhibited by a new dense capillary network within the tissue. Schumacher et al., "Induction of Neo-Angiogenesis in Ischemic Myocardium by Human Growth Factors", *Circulation*, 1998; 97:645-650. The authors noted that such treatment could be an approach to management of diffused coronary heart disease after alternative methods of
20 administration have been developed.

Summary of the Invention

The present invention provides a delivery system for placing implants within tissue in the human body. The implant delivery system of the present invention
25 provides several novel features, which are useful in delivering implants into tissue.

In one aspect of the invention a delivery device is provided that is especially configured to carry multiple tubular shaped implants at its distal end, engaging the implants by their inside surfaces. The delivery devices are inserted percutaneously into a patient and navigated to the site where the implant is to be located. The
30 delivery systems of the present invention are particularly well suited for delivering

- 4 -

implants into the myocardium to perform transmural revascularization (TMR). Implants such as stents may be placed by the delivery device into the myocardial tissue to a proper depth to encourage revascularization of ischemic tissue. In such a procedure, positioning the implants into the proper depth within the myocardium is
5 important to the success of the procedure because it has been observed that areas of the myocardium closer to the endocardial surface and to the epicardial surface are more likely to be responsive to revascularization. Additionally, spacing of the implants relative to one another in an area of ischemic tissue is important to the success of the revascularization process and avoiding undesirable side effects of placing foreign
10 objects in the muscle tissue of the myocardium. Additionally, it may be desirable to deliver a therapeutic substance to the implant location, before, after or during delivery of the implant to promote revascularization activity such as angiogenesis. The features of the present invention address these concerns as will be discussed in greater detail below.

15 Reaching the intended implant delivery location with the delivery devices of the present invention first requires placement of a guide catheter prior to navigation of a deliverable catheter into the left ventricle. A steerable catheter that is placeable within the left ventricle and positionable in multiple locations with one catheterization is disclosed in U.S. application serial no. 09/073,118 filed May 5, 1998, the entirety of
20 which is herein incorporated by reference. The delivery devices as described herein are insertable through the lumen of the delivery catheter and are extendible past its distal end to place the implants within the myocardial tissue. The delivery catheter provides directional control so that the delivery devices of the present invention can deliver multiple implants to a variety of locations within a given area of ischemic
25 tissue.

In one embodiment of a delivery device of the present invention the device comprises a catheter having a compressible sleeve at its distal end which forms into a plurality of random folds when it is compressed expanding its diameter and serving to capture the inside surface of any tubular object placed over it. The crinkle tube may
30 be formed from a polymer such as polyethylene terephthalate (PET). The crinkle tube

- 5 -

can securely retain tubular implants over its crinkle, radially expanded surface to a sufficient degree such that delivery into tissue does not push the implant off of the delivery device. Additionally, the crinkle tube catheter may be used in conjunction with an outer catheter shaft having a plurality of interior projections which engage a plurality of implants in cue while the crinkle tube shaft delivers the implants from the distal end of the catheter sequentially.

In another embodiment, a tubular implant is maintained on the catheter behind an oval shaped segment of the catheter which presents a larger profile than the inside diameter of the tubular implant. A member is slidable within the catheter engages the oval portion to deform into a round shape, thereby permitting the implant to slip off the distal end of the shaft. Simultaneously with deformation of the oval to a circle shape, the inner member causes arms to protrude from the interior of the catheter and to engage the implant and push it in a distal direction so that it becomes implanted in the tissue. Additionally, the catheter has the ability to carry multiple implants over its shaft. The implants waiting in cue are also maintained in position on the shaft by a oval shape segment of the shaft that can be deformed to a circular shape thereby permitting advancement of the next implant.

In yet another embodiment of the delivery system, the delivery catheter comprises an elongate shaft that contains pressurized fluid within its lumen to motivate a plunger located at the distal end of the shaft and attached to a single implant attachment device. When fluid within the lumen of the delivery catheter is pressurized, the plunger moves from its position against proximal stops distally to its position against distal stops. That length of travel is sufficient to push the implant attached to the plunger into the intended tissue location. The benefit of the fluid pressure delivery system is the reduction in moving components needed to cause distal movement of the implant at the distal end of the catheter from the proximal end of the catheter which is manipulated outside of the patient.

Another feature of the present invention includes a dual bladder drug delivery system which may be associated with the delivery catheters discussed above. The dual bladder arrangement provides a first bladder which contains a therapeutic

- 6 -

substance near the distal end of the delivery catheter and a second bladder arranged near the first bladder so as to impinge upon the space of the first bladder when the second bladder is inflated. The second bladder is inflated with an inexpensive fluid simply to cause the evacuation of the first bladder, which contains a therapeutic
5 substance to be delivered. The first bladder may be provided with a series of perfusion ports through which the therapeutic substance can be forced through when pressurized by the reducing volume imposed by the inflation of the second bladder. The benefit of the system is to avoid the waste of expensive therapeutic substances by filling an entire full length lumen with the substance in order to force it from the
10 distal end of a delivery catheter. With the dual bladder delivery system, an expensive fluid can be used to occupy the space along the full length of the delivery catheter, yet its pressurization force can be applied to deliver a small quantity of the therapeutic substance maintained only at the distal end of the catheter.

Another feature of the present invention is a depth monitor, which may be
15 applied to any of the above delivery catheters. The depth monitor uses changes in pressure being measured at the distal end of the catheter to signal the operator that the distal end of the catheter has been placed within myocardial tissue to a certain depth sufficient to implant the device. This depth monitoring is accomplished by providing one or a plurality of pressure ports at the distal end of the catheter that will
20 be inserted into tissue in order to deliver the implant that it carries. The pressure port(s) are spaced a known distance from the distal end of the delivery catheter. The interior lumen of the catheter can transmit the pressure experienced at the distal end of the catheter through individual lumens to the proximal end where a pressure monitoring device for each pressure port is attached to the proximal end of the
25 delivery device. When the distal end of the delivery catheter is in the left ventricle, pressure readings at the distal end will be dynamic. However, after the distal end of the delivery catheter enters the tissue to implant the device, the pressure ports become covered with surrounding tissue resulting in dampened or static signal. The most proximal pressure port when covered by the surrounding tissue, will act likewise

- 7 -

and signals the operator that the distal end of the delivery catheter has been placed to a sufficient depth within the tissue to deliver the implant.

Another feature of the present invention is a navigation system utilizing magnetic fields transmitted over the body to identify the location within a patient of a catheter having sensing electrodes that interact with the electromagnetic coils.
5 Computer software processes the information obtained from the magnetic pick-up coils and places the catheter on a virtual image of the heart to give the operator a general idea of where the catheter is located and what areas of ischemic tissue have been treated with implant devices. Because the delivery devices of the present
10 invention are capable of delivering more than one implant to an area of ischemic tissue with one catheterization, a navigation system helping to guide the placement of the delivery catheter and implants is helpful.

It is an object of the present invention to provide an implant delivery system that is simple and effective to use. It is yet another object of the present invention to
15 provide an implant delivery system that is suitable for varying implant devices to the myocardium of the heart that will aid in revascularization of ischemic tissue.

It is yet another object of the invention to provide an implant delivery device that operates to grasp a tubular shaped implant by its inside surface. The implant may be inserted into tissue. It is another object of the invention to provide an implant
20 delivery device that utilizes fluid pressure through the delivery catheter to insert the implant into the subject tissue.

It is yet another object of the invention to provide an implant delivery device that includes a dual bladder drug delivery system that reduces waste of expensive therapeutic substances in its application to a treatment site through a catheter.

25 It is still another object of the invention to provide a depth monitor capable of being associated with a delivery device that utilizes pressure sensed at the distal end of the catheter to reliably determine the location of the distal end of the device.

It is yet another object of the invention to provide a navigation system that is capable of identifying the location of a catheter delivering mechanical TMR inducing

devices, within the human heart so that the catheter can be moved to various locations delivering multiple devices with one insertion into the heart.

Brief Description of the Drawings

5 The foregoing and other objects and advantages of the invention will be appreciated more fully from the following further description thereof, with reference to the accompanying diagrammatic drawings wherein:

FIG. 1 shows a sectional illustration of the left ventricle of a human heart;

10 FIG. 2 A- 2D illustrate the steps of percutaneously delivering an implant to an area of the myocardium;

FIG. 3A is a partial sectional illustrational of the crinkle tube delivery device;

FIG. 3B is a detail of the crinkle tube in compression;

FIG. 3C is a detail of the crinkle tube in tension;

15 FIG. 3D is a partial sectional illustration of the crinkle tube device delivering an implant;

FIG. 3E is a partial sectional illustration of the crinkle tube device being withdrawn from the implant location;

FIG. 3F is a partial sectional illustration of a delivery device having a depth monitor;

20 FIG. 4A-4C are partial sectional illustrations of a multiple implant device;

Fig. 5A is a partial sectional view of a oval tube delivery device;

FIG. 5B is a sectional view taken along the line 5B-5B of FIG 5A;

FIG. 5C is a sectional view taken along the line 5C-5C of FIG 5A;

FIG. 6A is a partial sectional view of an oval tube delivery device;

25 FIG. 6B is a sectional view taken along the line 6B-6B of FIG. 6A;

FIG. 6C is a sectional view taken along the line 6C-6C of FIG. 6A;

FIG. 7A is a partial sectional view of an oval tube delivery device;

FIG. 7B is a sectional view taken along the line 7B-7B of FIG. 7A;

FIG. 7C is a sectional view taken along the line 7C-7C of FIG. 7A;

- 9 -

FIG. 8 is a sectional view of a pressurized fluid delivery device;

FIG. 9A is a sectional view of a double bladder therapeutic substance delivery device;

FIG. 9B - 9C are sectional views of the double bladder therapeutic substance
5 delivery device.

Description of the Illustrative Embodiments

10 FIG. 1 shows a sectional illustration of the left ventricle 2 of a human heart 1. Several implants 8 are placed within the myocardium 4 adjacent the endocardial surface 6. As shown in FIGS. 2A-2D, access to the endocardial surface 6 of the myocardium 8 is gained through a steerable delivery catheter 36 inserted into the left ventricle 2. It is through the delivery catheter 36 that the delivery devices of the
15 present invention are inserted to carry the individual implants into the myocardial tissue 8. The steerable delivery catheter 36. It is noted, throughout the description of the delivery devices and their associated methods, "proximal" refers to the direction along the delivery path leading external of the patient and "distal" refers to the direction leading internal to the patient.

20 To access the left ventricle of the heart percutaneously, a guide catheter (not shown) may be navigated through the patient's vessels to reach the left ventricle 2 of the heart 1. A barbed tip guidewire 34 may then be inserted through the guide catheter and into the ventricle where it pierces the myocardium 4 and becomes anchored within the tissue. After anchoring the guidewire, the steerable delivery
25 catheter 36 may be advanced over the guidewire to become positioned within the ventricle in close proximity to the endocardium to facilitate delivery of implants. To facilitate delivery of multiple implants, the guidewire lumen of the delivery catheter 36 may be eccentrically located on the catheter. Therefore, when the catheter is rotated about the guidewire, the center of the catheter will rotate through a circular path as
30 demonstrated in FIGS. 2C and 2D, to encompass a broader delivery area with only a

- 10 -

single guidewire placement. The outside diameter of the delivery catheter is preferably less than .100 inch. Additionally, the delivery catheter may be provided with steering capability by means of a pull wire extending the length of the catheter and attached at its distal end such that pulling on the wire from the proximal end
5 causes the distal tip of the catheter to be deflected. Therefore, the steering capability provides a broader range of delivery area with a single catheterization. A detailed description of the construction of a delivery catheter for reaching multiple sites within the left ventricle is described in U.S. patent application serial no. 09/073,118 filed May 5, 1998, the entire disclosure of which is herein incorporated by reference.

10 FIG. 3A shows a partial cut-away view of a preferred delivery device 10 for the TMR implants 8. The delivery device 10 shown in FIG. 3A may be used with a guide catheter 12 rather than the steerable catheter 36 discussed above. A delivery device 10 comprises an elongate solid shaft 14 having a sharp obturator head 16 at its distal end. The obturator head 16 is formed at the distal end of the core wire 14 by any
15 convenient means of building a mass at the end of a core wire. For example, several thin and small sleeves and springs may be amassed at the distal end and melted together to form a bulbous tip which is later ground to form a sharp, piercing tip 18. Included within the mass of melted materials that form the distal obturator head 16, should be a radiopaque material such as gold or platinum to make the distal area of
20 the device visible under fluoroscopy. Heat bonded to the proximal end 20 of the obturator head 16 is a flexible crinkle tube 22, shown in detail in FIG. 3B, formed from polyethylene terephthalate (PET). Attached to the proximal end 24 of the crinkle tube 22 by heat bonding is push tube 26 which is formed from a closely wound spring having a PET shrink tube formed around its outer surface filling in the voids created by
25 the coils. The crinkle tube 22 collapses under compressive load to form a random pattern of folds 28, which serve to increase the overall diameter of the crinkle tube such that it comes into frictional contact with the inside diameter of a hollow or generally tubular implant 8 that is placed over it. When placed in tension as shown in FIG. 3C, the crinkle tube elongates and returns to a low diameter configuration
30 without folds. The configuration of the crinkle tube is manipulated by relative

- 11 -

movement of the core wire 14 having its obturator 16 joined to the distal end 25 of the crinkle tube relative to the push tube 26, which is joined to the proximal end of the crinkle tube 24. The shaft and push tube are slidable relative to each other and controllable from the proximal end of the device by a handle 38 and core wire extension 30. Movement of the handle and push tube in a distal direction and movement of the core wire and its extension in the proximal direction compress the crinkle tube 22 to capture the interior of an implant 8 for delivery into tissue as shown in FIG. 3A. It is in this large diameter, crinkled configuration that the delivery device must maintain to restrain the implant during delivery into tissue. As shown in FIG. 3D and 3E after delivery into tissue, the crinkle tube may be placed in tension, to withdraw the plurality of folds that engage the interior of the implant 8. With the crinkle tube 22 placed in a low profile configuration, the core wire extension 30 is advanced distally within the handle 38 and handle 38 advanced distally into the associated guide catheter 12 as shown in FIG. 3D. After reducing the profile of the crinkle tube 22 the implant easily slides off of the crinkle tube 22 over the obturator 16 as the device is withdrawn from the tissue as shown in FIG. 3E.

An alternative embodiment of the crinkle tube delivery device may be additionally equipped with a pressure dependent depth monitor. The depth monitor may be comprised of at least one pressure port 21, shown in FIGS. 3B and 3F, formed in the push tube 26 adjacent its distal end 27 and location of the crinkle tube 22 and implant. Pressure sensed through the port 21 is transmitted through lumen defined by the push tube and is detected by a pressure detector 31 joined to the handle 38. Readings from the pressure detector may be shown on a hydraulic gauge or electronic readout.

The location of the pressure port 21 is a significant factor in interpreting the pressure information for proper implant delivery. When the pressure port is open to the left ventricle, pressure readings are dynamic. However, when the pressure port 21 is submerged and covered by tissue, pressure readings drop or become static. With placement of the pressure port just proximal of the implant mounting location on the push tube, a significant pressure dampening during delivery of an implant will

- 12 -

signal the operator that, not only has the pressure port become embedded in the tissue, but also the implant, located distal to the pressure port, has become sufficiently imbedded in the tissue. Thus the implant can be released from the delivery device and into the tissue. Multiple pressure ports spaced along the distal end of the delivery device can provide an indicator of how deep the delivery device is in the tissue because as each successive pressure is monitored.

FIG. 4A shows a variation of the crinkle tube delivery device, which is configured to sequentially delivery several preloaded implants 8. The multiple implant delivery device 34 operates much the same way as the single implant delivery device described above. The crinkle tube 22 grips the most distal implant 8 only, while the other implants wait in cue within the guide catheter 12 and over the push tube 26. The additional implants are restrained in their relative positions behind the most distal implant by resilient fingers 44 which project inwardly from the interior wall 46 of guide catheter 12. After the most distal stent is urged out of the guide catheter by the distal movement of the core wire and push shaft, as shown in FIG. 4B, the core wire and push shaft may be retracted back into the guide catheter as the remaining stents are indexed distally by the sliding distal movement of index cue 40 which may be manually slidable within the guide catheter 12 by indexing shaft 42. As the core wire 14 and push tube 26 are withdrawn proximally back into the guide catheter, the area of the crinkle tube 22 resides in the interior of the newly placed most distal stent. The push tube and core wire are again moved relative to each other to cause compression along the crinkle tube 22 so that the folds 28 of the crinkle tube 22 contact the interior surface of the next implant 8 to be delivered. The next implant to be delivered is preferably placed in a different location, spaced apart from the first implant by movement of the guide catheter 12 to a new area.

FIGS. 5A-C shows another embodiment of the implant delivery device 50. The device operates to maintain an implant 8 over its outer shaft 54 by having a distal oval area where the shaft defines an oval cross-sectional shape, as shown in FIG. 5B, that defines a diameter that is larger than the circular shape of the tubular implant 8, to thereby preventing the implant from sliding off the end of the outer shaft 54.

- 13 -

Additionally, the proximal oval area 68 on the outer shaft 54 maintains the implant 8 that is second in line in its mounted configuration on the catheter shaft. The natural tendency of the shaft 54 to maintain an oval shape at these areas serves to lock the implants 8 in place on the shaft as is shown in FIG. 5A. It is in this locked
5 configuration that the most distal implant is navigated to the myocardium. The oval areas of the outer shaft 54 lock the implants in place so that they do not move as they are navigated to the tissue location.

FIGS. 6A-C shows an implant 8 being delivered from the oval shaft
embodiment 50. Once the delivery device is adjacent the tissue to be penetrated, the
10 shaft 52 is advanced distally causing the sharpened distal tip 70 of the shaft to emerge from the distal end 72 of the delivery device. The sharpened distal tip 70 pierces tissue as it is advanced in a distal direction to facilitate insertion of the implant 8 into the tissue. Also with the distal movement of the shaft 52, the distal cam 56 moves into engagement with the distal shims 62, thereby causing the naturally oval
15 area 66 to be elastically deformed into a round shape as is shown in FIG. 6B. The round configuration of the outer shaft 54 in this area permits the round implant to slide off the distal end of the device. Further distal movement of the shaft 52 causes distal movement of the split tube 76, which is engaged by the proximal cam 60 joined to the shaft 52. The vanes 78 of the split tube move distally and curve radially outward
20 through radial passages 80 formed into the sidewall of the outer shaft 54 to engage the interior of the most distal implant. The natural curvature of the vanes and the presence of biasing member 84 underneath the vanes urge them in a radially outward direction so that as they are moved distally within the shaft 54 the vanes are urged out of the radial passages 80 that are formed in the tube. Though the vanes serve to
25 push the implant into the desired tissue location, their radial extent from the catheter shaft 54 could potentially interfere with the passage of the proximal end 9 of the implant over the vanes. Therefore, to ensure that the implants are not hindered as they are pushed off the catheter shaft, the implants used with the present embodiment of delivery device should be configured to have a proximal opening that

- 14 -

is larger than the distal opening and as large as the maximum extent of the natural extent of the vanes. .

During delivery into the myocardium the proximal oval area 68 is maintained in the oval configuration to lock in place on the shaft 52 the implants 8 that are in cue to be delivered. However, after delivery of an implant into tissue, the shaft is retracted proximally within the shaft 54 to shield the sharp distal tip 70 from tissue during movement of the shaft to the next location, as shown in FIG. 7A. Distal movement of the shaft 52 also causes the proximal cam 60 to engage the proximal shim 62 located on the inner surface of the outer shaft lumen directly adjacent the proximal oval area 68, which forces the shaft to become circular temporarily in that area, as shown in FIG. 7C. Thus the secondary implants become free to cue forward, the next implant 8 moving up to be the next delivered. The arrangement of cams on the shaft dictates that when the proximal oval area is deformed to be round, the distal oval area remains in its undeformed oval configuration to prevent continued distal movement of implants 8 distally on the shaft until they are ready to be delivered into tissue.

FIG. 8 is partial sectional view of another embodiment of the delivery device of the present invention that uses pressurized fluid to provide the implantation force needed to insert a self-piercing stent into myocardial tissue. The fluid pressure delivery device 90 comprises an elongate shaft 92 having at least one lumen 94, which carries the pressurized fluid 96 such as water or saline. The fluid and a pressurization source are joined to the lumen at proximal luer fitting 98. The shaft may have a guidewire lumen 99 containing a barbed tip guidewire 34, as with the delivery catheter 36 described above. The barbed tip guidewire implanted within adjacent tissue helps provide leverage to resist movement of the distal tip 100 of the catheter when when substantial fluid force is being applied to the tissue surface by the entering implant 8.

The distal portion 102 of the lumen 94 is configured as a track 104 to receive a slidable plunger 106 that forms a fluid tight seal with the track. Fluid pressure within the lumen 94 creates a force against the plunger causing it to slide distally. The plunger has joined to its distal face a catch member 108 that is configured to be

- 15 -

releasably engagable with the interior of an implant 8 with which the device is intended to deliver into tissue. The extent of travel of the plunger within the track 104 is limited by proximal stops 110 and distal stops 112 that engage the plunger to limit its movement so that it does not become disassociated from the shaft lumen 94 when travel is maximized. To avoid the necessity of attaching a piercing member to the plunger, self-piercing implants are preferred for use with the present embodiment, such as shown in FIG 8. Examples of self piercing implants intended for placement in the myocardium are described in U.S. Patent Application Serial No. 09/073,118, filed May 5, 1998.

Figure 9A - 9C show a double bladder therapeutic substance delivery system 110 that may be employed with the implant delivery systems of the present invention that can be configured to have an open lumen through their lengths. In particular the crinkle tube 22 and oval shaft 50 embodiments may be configured to employ the therapeutic substance delivery system 110. Figure 9A shows a double bladder system 110 positioned within the central lumen 112 of a tube 111 of an implant delivery system similar to the crinkle tube delivery device. It is noted that other implant delivery systems or catheter devices not disclosed herein may employ the therapeutic substance delivery system or the system could be deployed alone through a conventional catheter having a lumen.

The drug delivery system shown in FIGS. 9A - 9C employs a first flexible bladder 114 filled with a therapeutic substance and mounted about a tube, 116 and in close longitudinal proximity to (FIG. 9B), or surrounding (FIG. 9C) a second flexible bladder 118 attached to the shaft 116 and inflatable with a conventional medium such as saline. The second bladder 118 is in fluid communication with a lumen 120 that extends through shaft 116 via a port 122. Expansion of the second bladder 118 within a confined space such as within a lumen 112 adjacent the first bladder 114 (FIG. 9B) or from within the first bladder (FIG. 9C) applies pressure to the first bladder, reducing its volume which increases fluid pressure in the first bladder sufficiently to cause the therapeutic substance to be ejected through tiny orifices 124 to the intended treatment site.

- 16 -

The bladders may be similar to dilatation balloon in their shape, size and manner of attachment to the shaft 116. The bladders may be made from a strong but flexible material such as PVC or Nylon. The bladders may be approximately the same size so that volume reduction of the first bladder corresponds to the volume expansion of the second bladder. The first bladder may be filled with a therapeutic substance during the process of joining it the bladder to the shaft. After bonding the proximal neck 130 to the shaft, the catheter may be oriented so that the distal neck 132 is elevated. In this orientation, the therapeutic substance can be injected, by a syringe, inserted between the distal neck and the shaft, without the chance of the substance running out of the bladder or contaminating the bonding area between the distal neck and the shaft. After filling the bladder 114 with the substance, the distal neck is bonded to the shaft.

A plurality of tiny orifices 124 may be preformed in the drug bladder prior to use of the device and either prior or after being filled with the substance and bonded. Because the orifices are small, on the order of .001", and the substance within the first bladder is not pressurized it is expected that most therapeutic substances can be formulated to have a sufficiently high viscosity that the substance will not leak out from the orifices in the absence of pressure applied by the second bladder. For this reason, an alternative method of prefilling the first bladder with a therapeutic substance may comprise the steps of piercing the surface of a bladder with a tiny syringe needle and injecting the substance through the bladder wall.

Another aspect of the invention utilizes electromagnetic guidance technology to provide a guidance system for use with an implant delivery system such as the systems discussed above. U.S. Patent No. 5,769,843 (Abela), the entirety of which is incorporated herein by reference, discloses such a guidance system for positioning a laser catheter within the ventricle of the heart. An electromagnetic guidance system would be especially useful in the delivery of multiple mechanical implants to an area of ischemic myocardial tissue such as is described above. The delivery devices of the present invention may be equipped with two non-coplanar magnetic sensing coils in the distal ends of their shafts to cooperate with three sets of three magnetic fields

- 17 -

generating external coils located outside the patient. The sensing coils of the catheter receive the electromagnetic field and thus, with assistance with from a computer can be located within the patient.

From the foregoing, it will be appreciated that the invention provides delivery
5 devices for delivering implants and therapeutic substances to the myocardium. The invention is particularly advantageous for delivering devices and therapeutic substances to promote TMR and angiogenesis within ischemic myocardial tissue. The implants are simple and readily insertable into the intended tissue location with a minimum of steps. The delivery systems are simple to operate to implant the devices
10 quickly.

It should be understood, however, that the foregoing description of the invention is intended merely to be illustrative thereof and that other modifications, embodiments and equivalents may be apparent to those skilled in the art without departing from its spirit. Having thus described the invention what we desire to claim
15 and secure by letters patent is:

CLAIMS

1. A delivery device for a hollow implant comprising:
an elongate shaft having proximal and distal ends and a lumen ;
5 at least one deformable surface adjacent to the distal end that can be
deformed to contact an inside surface of an implant and reformed to release the
implant.
2. An implant delivery device as defined in claim 1 wherein the deformable
10 surface is common with the shaft.
3. An implant delivery device as defined in claim 3 wherein the deformable
surface is a section of the shaft having an oval cross sectional shape that is
deformable to have a circular cross-sectional shape.
15
4. An implant delivery device as defined in claim 3 further comprising:
a cam slidable within the lumen of the shaft that is selectively
engageable with the oval sections to deform them to a round cross-sectional shape.
- 20 5. A method of implanting an implant device in the human body
comprising:
providing a shaft generally circular in cross-sectional shape, having a
lumen and proximal distal ends and at least one segment having an oval cross-
sectional shape;
25 placing a tubular implant over the shaft such that the inside diameter of
the tube becomes caught on the oval section of the shaft;
navigating the shaft and associated implant tube to the intended delivery
site within a patient;
deforming the oval segment to circular cross-sectional shape to permit
30 the tubular implant to slide over the segment and off the shaft.

- 19 -

6. An implant delivery device as defined in claim 1 further comprising:
a collapsible sleeve having a proximal end and a distal end and being
mounted around the distal end of the shaft defining the deformable surface.

5

7. An implant delivery device as defined in claim 6 further comprising:
a push tube mounted over the shaft and slidable relative to the shaft and joined to
the proximal end of the sleeve such that longitudinal movement of the push tube
relative to the shaft places an axial load on the sleeve.

10

8. An implant delivery device as defined in claim 7 wherein movement of
the push tube in a distal direction relative to the shaft places the sleeve in axial
compression resulting in collapse of the sleeve and the formation of multiple folds
having peaks that define a diameter that is larger than the diameter of the unloaded
sleeve.

15

9. A method of implanting an implant device in the human body
comprising:

providing a shaft having a distal end and a collapsible sleeve having a
surface mounted around its distal end;

20

placing a hollow implant over the collapsible sleeve;
placing an axial load on the sleeve to collapse it and cause the formation of a plurality
of folds along its surface thereby engaging the interior of the implant;

25

navigating the shaft and associated implant tube to the intended delivery
site within a patient;
placing the sleeve in tension to remove the folds and release the implant
from engagement with the implant.

10. An implant delivery device comprising :

- 20 -

A tubular shaft having a lumen and proximal and distal ends;
a plunger having a proximal side and a distal side configured to hold an
implant and the plunger being in slidable and fluid tight engagement with the lumen at
the distal end of the shaft such that pressurization of fluid contained within the lumen
5 causes the plunger to move in a distal direction.

11. An implant delivery device as defined in claim 10 further comprising:
A pullwire joined to the distal end of the tube and extending proximally
through the proximal end and arranged such that placing the wire in tension causes
10 the distal end of the shaft to be deflected away from the axis defined by the shaft.

12. An implant delivery device as defined in claim 9 further comprising: a
source of pressurized fluid in fluid communication with the proximal end of the shaft.

15 13. A method of delivering an implant comprising:
providing a tubular shaft having a lumen and proximal and distal ends;
a plunger having a proximal side and a distal side configured to hold an
implant and the plunger being in slidable and fluid tight engagement with the lumen at
the distal end of the shaft;
20 placing an implant on the distal side of the plunger;
navigating the distal end tubular shaft and implant through a patient's
vasculature to an implantation site;
connecting the proximal end of the shaft to a source of fluid to be
pressurized:
25 filling the lumen with fluid and pressurizing the fluid to cause distal
movement of the plunger to drive the implant into the intended implantation site.

14. An implant delivery device comprising:
an outer delivery shaft having a lumen;

- 21 -

an inner shaft having a lumen

a first bladder with perfusion ports sealed around the shaft, defining an interior with a volume and containing a therapeutic substance within the interior and; a second bladder sealed around the shaft in close proximity to the first bladder and in fluid communication with the lumen.

5

15. An implant delivery device as defined in claim 14 wherein the second bladder is laterally displaced from the first bladder a minimal distance such that inflation of the second bladder causes significant contact with the first bladder so that deformation of the first bladder occurs.

10

16. An implant as defined in claim 14 wherein the second bladder is located within the interior of the first bladder such that inflation of the second bladder causes expulsion of the therapeutic substance through the perfusion ports.

15

17. A method of delivering an implant and a therapeutic substance to a treatment site within a patient comprising:

providing a shaft having a lumen, proximal and distal ends,

an inner tube within the shaft lumen having a lumen and a first bladder

20 having a volume and perfusion ports and containing a therapeutic substance and a second bladder in fluid communication with the tube lumen, and

an implant releasably attached to the distal end of the shaft;

navigating the shaft, tube and implant to the implantation site within a patient;

25 releasing the implant at the implantation site;

inflating the second bladder to reduce the volume of the first bladder and cause expulsion of the therapeutic substance in the area of the released implant.

30

18. A delivery system for implanting a device in tissue in a patient comprising:

- 22 -

a shaft having proximal and distal ends and means for temporarily restraining an implant at the distal end;

a depth monitor mechanism having a sensor at the distal end of the shaft and indicator means joined to the proximal end of the shaft.

5

19. A delivery system for implanting a device in tissue in a patient as defined in claim 18 wherein the depth monitor operates by sensing pressure at the distal end of the shaft.

10

20. A delivery system for implanting a device in tissue in a patient as defined in claim 19 further comprising :

a plurality of sensors spaced longitudinally along the shaft adjacent the distal end.

15

21. A method of monitoring the placement depth of an implant delivery device within tissue comprising:

providing an implant delivery device having proximal and distal ends and a plurality pressure sensors each, with independent output, longitudinally spaced and placed at known distances along the shaft;

advancing the distal end shaft into tissue;

20

observing which sensors record a pressure change in conjunction with the known placement of the sensors on the shaft to determine the position of the shaft.

22.. An implant delivery system for placing a device in a patient comprising:

a shaft having proximal and distal ends;

25

a mechanism for releasably retaining an implant at the distal end of the shaft;

a navigation system having components internal and external to the patient including sensors mounted on the shaft.

23. A catheter for accessing the left ventricle of the heart to promote revascularization of the myocardium by mechanical means comprising:

30

- 23 -

- an implant configured to promote revascularization of myocardial tissue
 - a shaft having proximal and distal ends;
 - a mechanism for releasably retaining the implant at the distal end of the shaft;
 - a navigation system having components internal and external to the patient
- 5 including sensors mounted on the shaft.

1/8

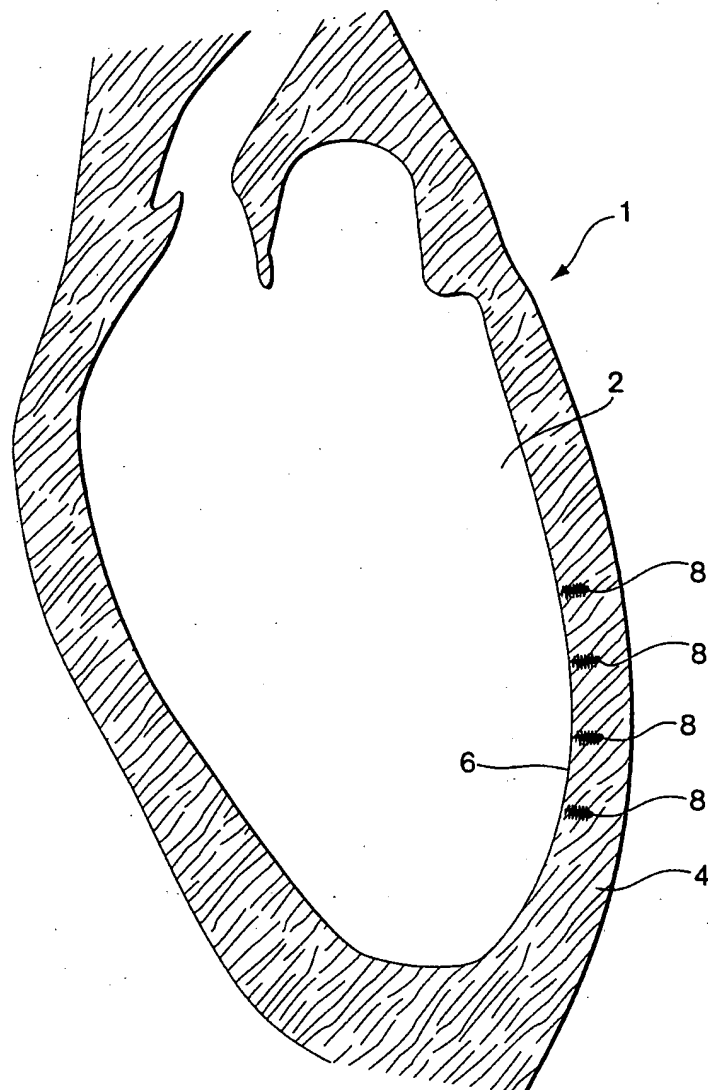


Fig. 1

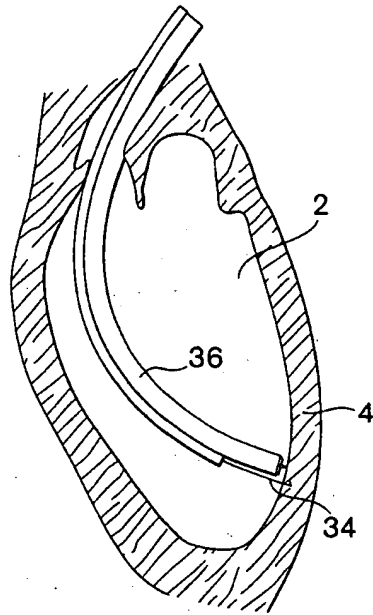


Fig. 2A

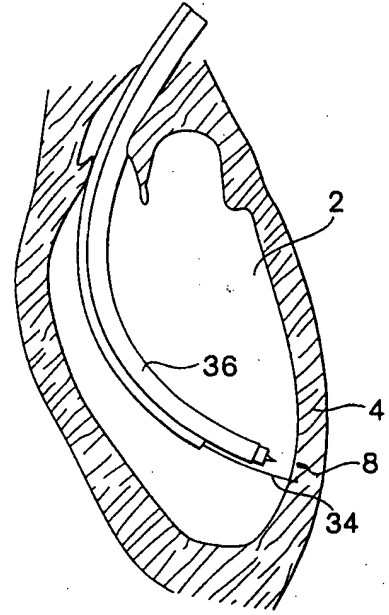


Fig. 2B

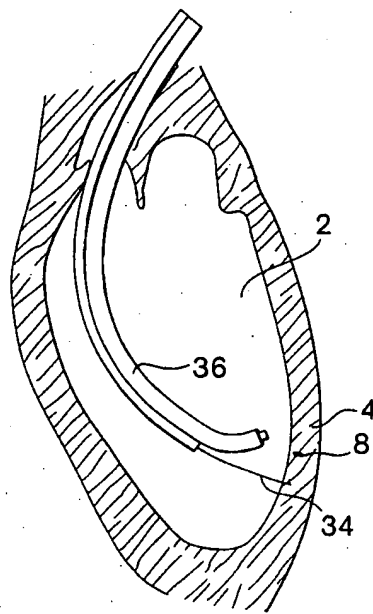


Fig. 2C

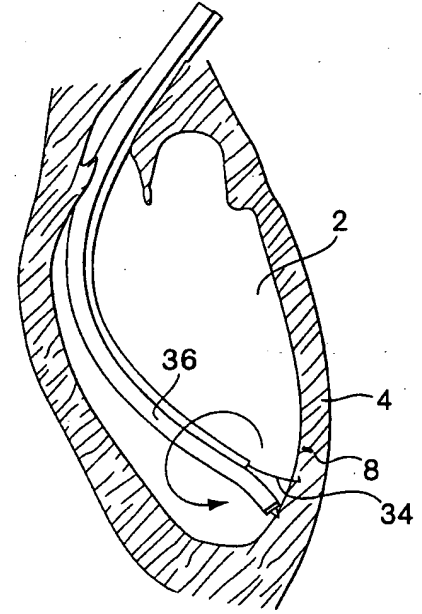


Fig. 2D

3/8

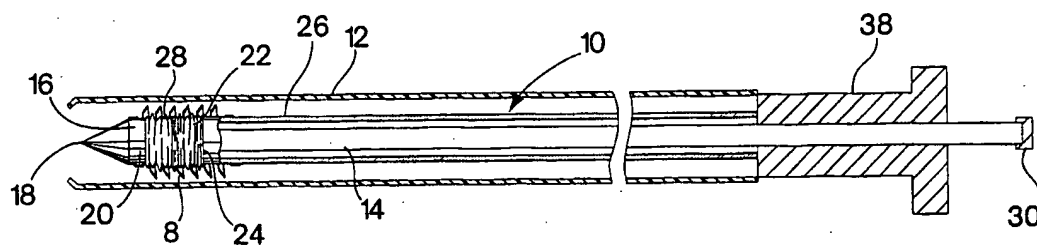


Fig. 3A

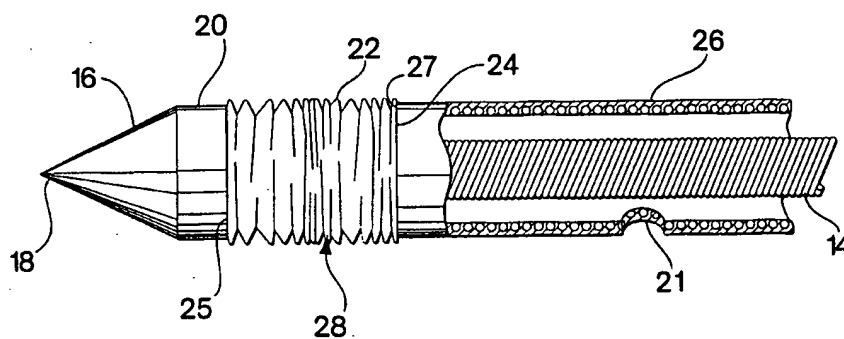


Fig. 3B

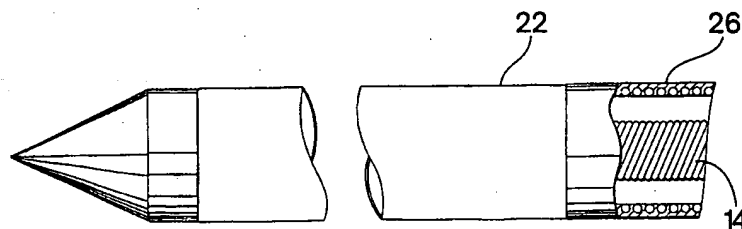
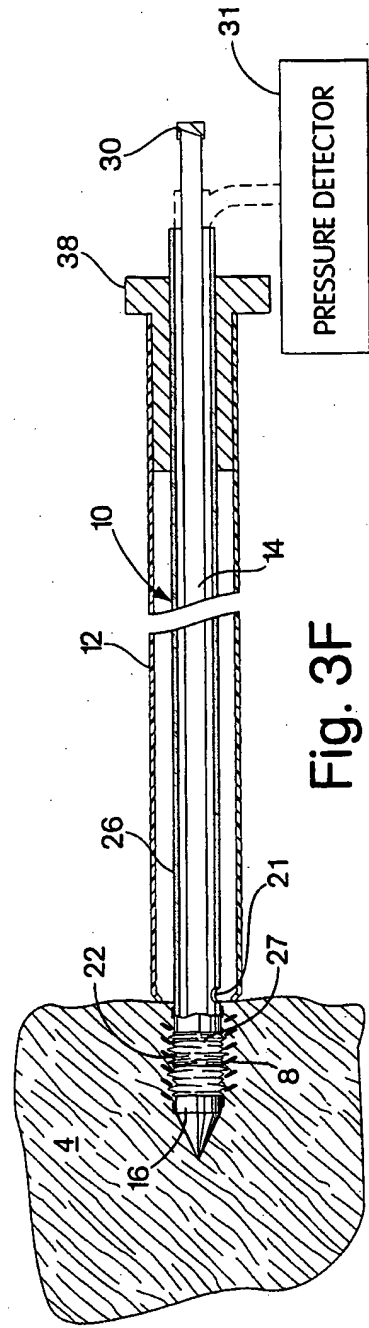
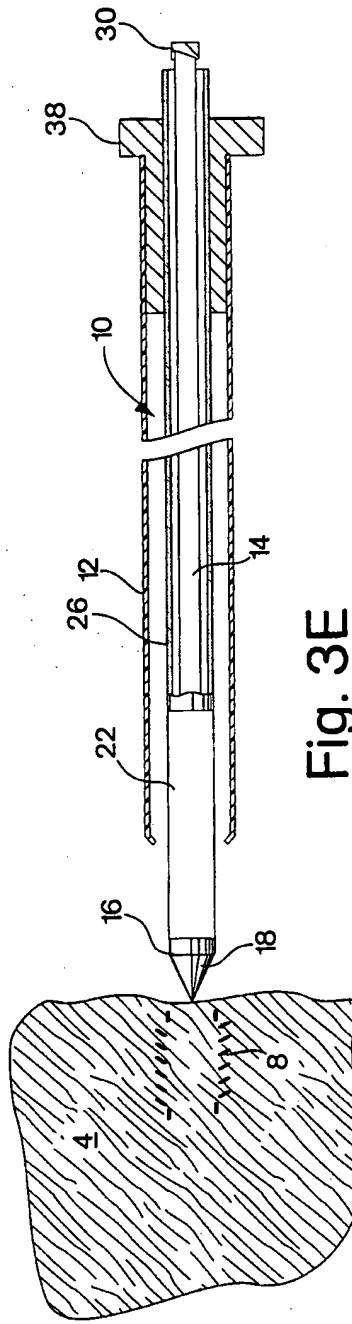
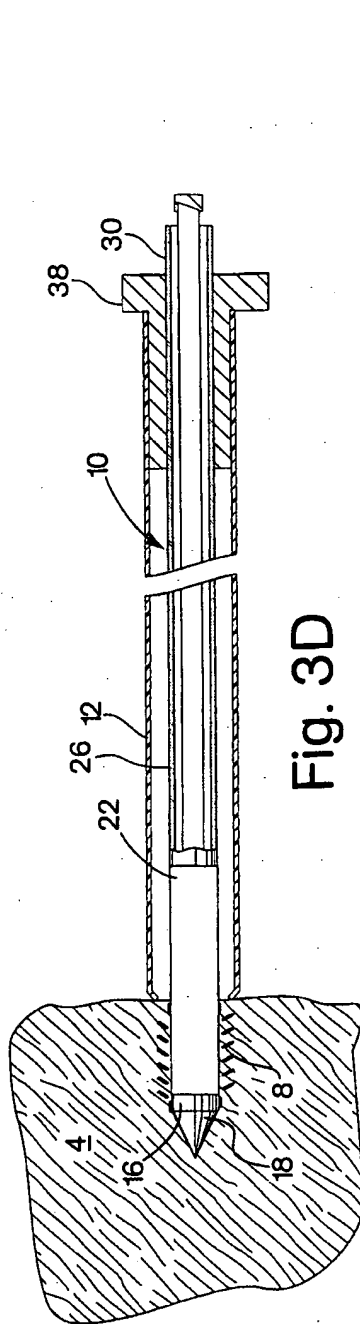


Fig. 3C



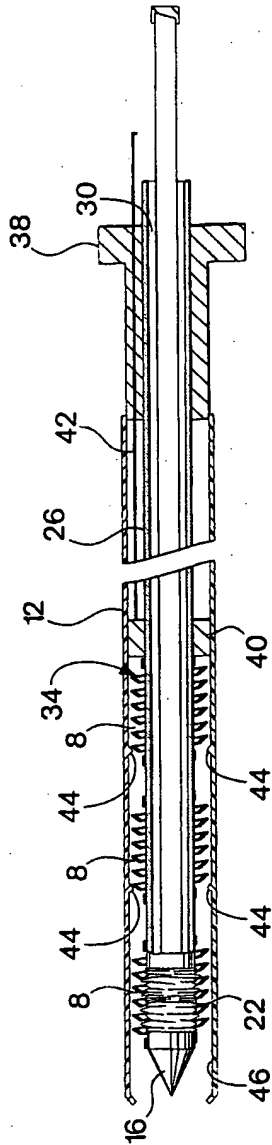


Fig. 4A

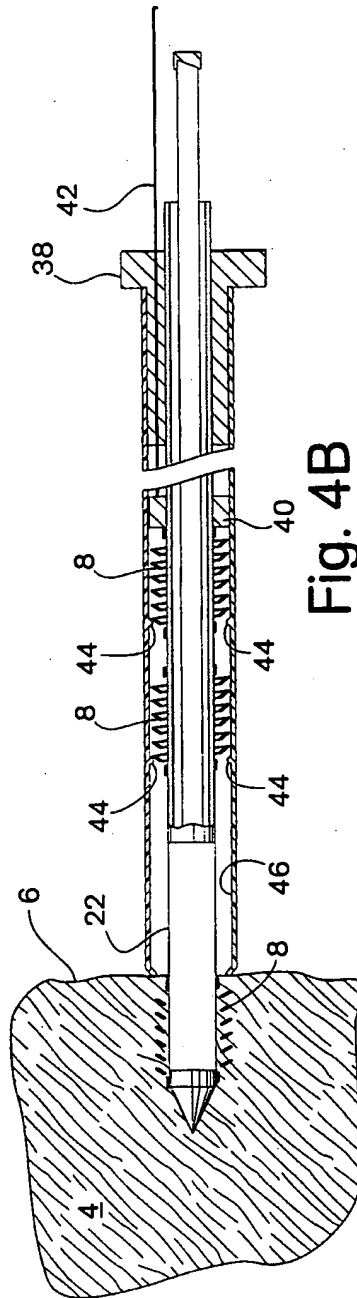


Fig. 4B

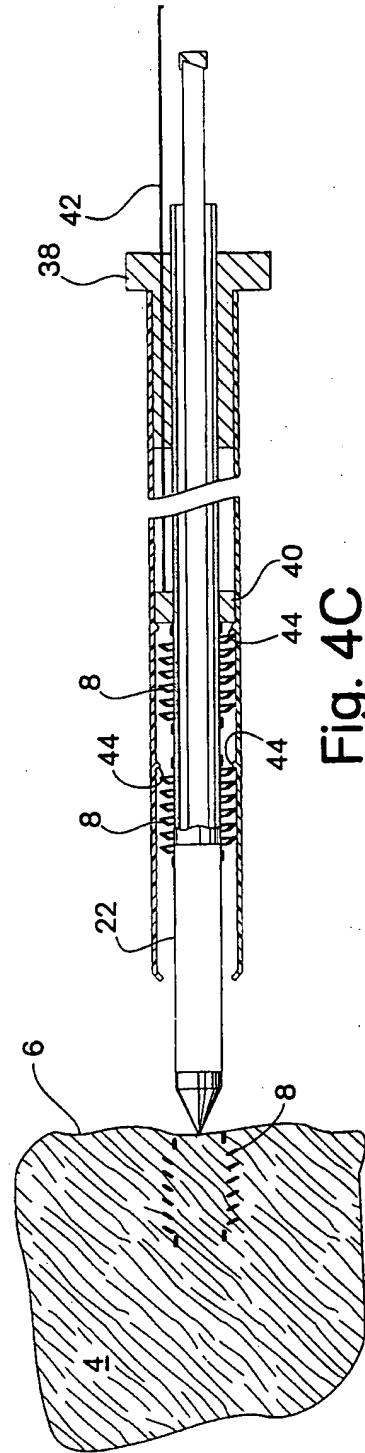


Fig. 4C

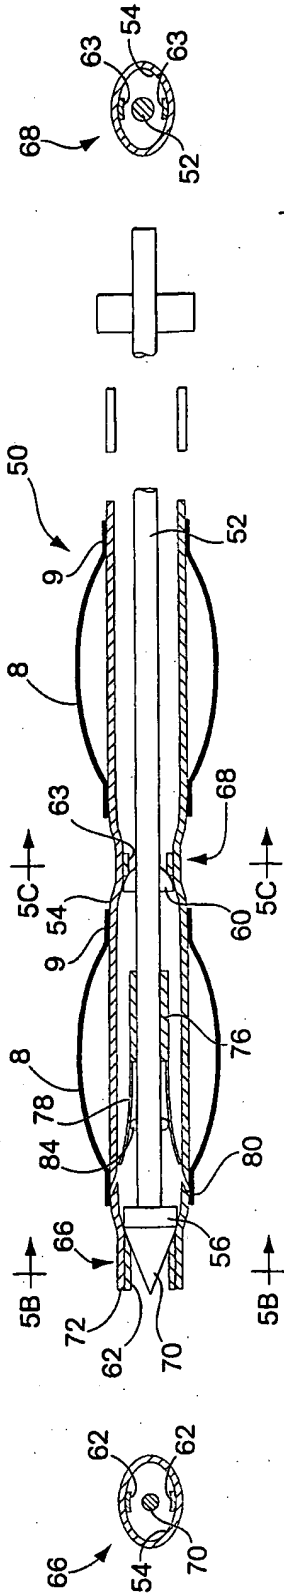


Fig. 5A

Fig. 5B

Fig. 5C

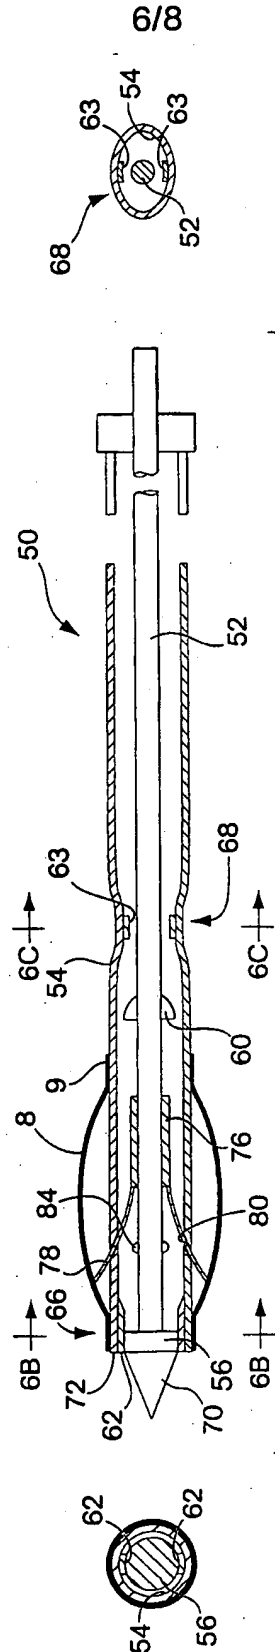


Fig. 6A

Fig. 6B

Fig. 6C

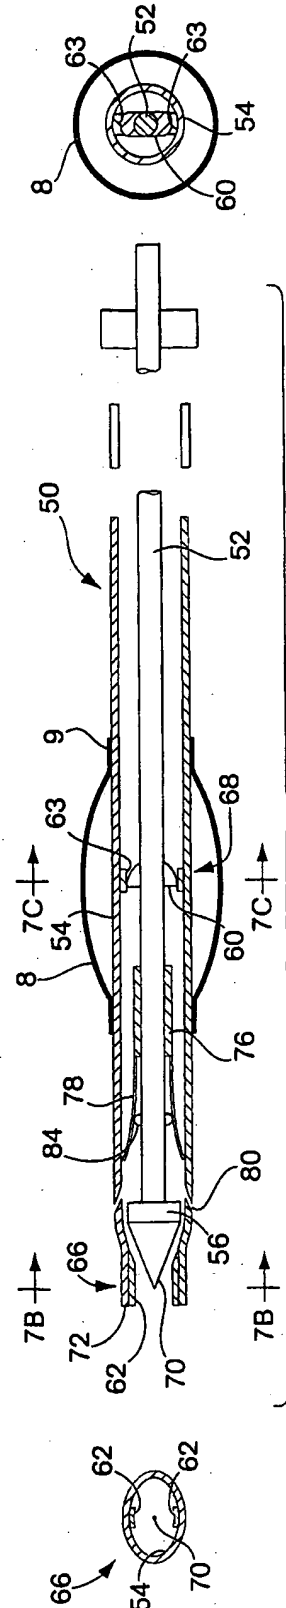


Fig. 7A

Fig. 7B

Fig. 7C

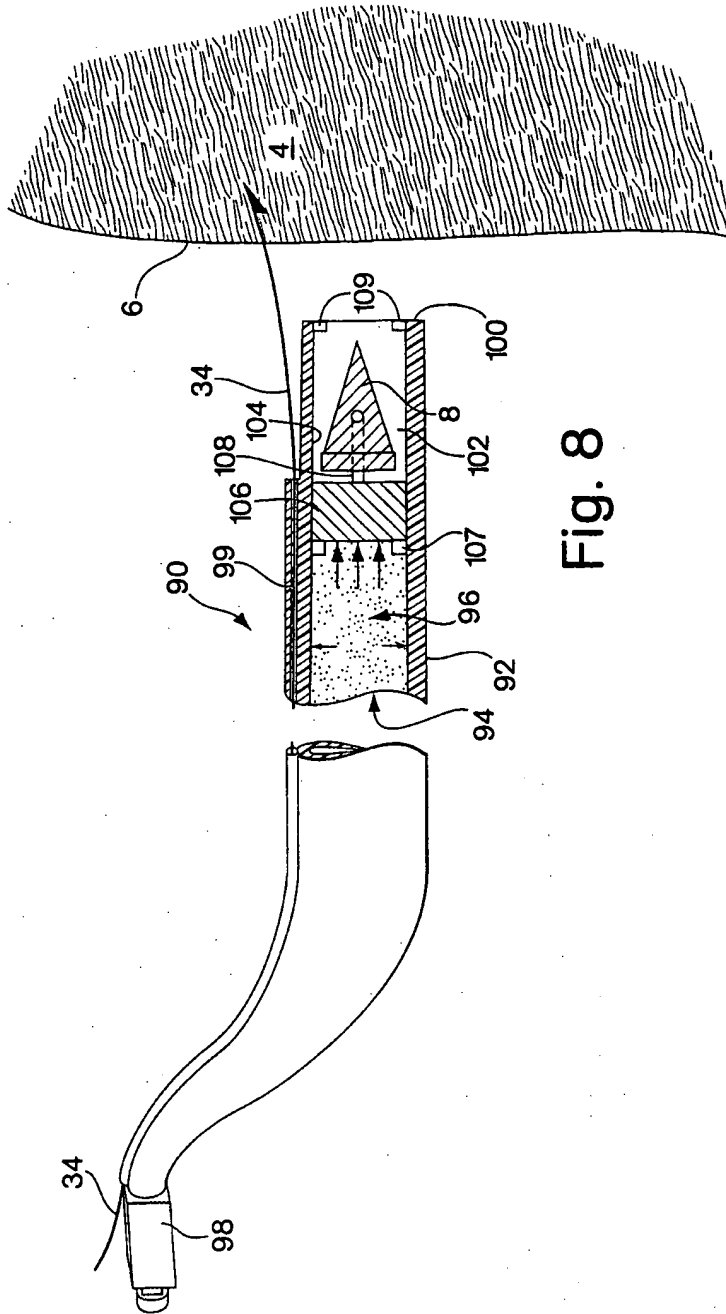


Fig. 8

8/8

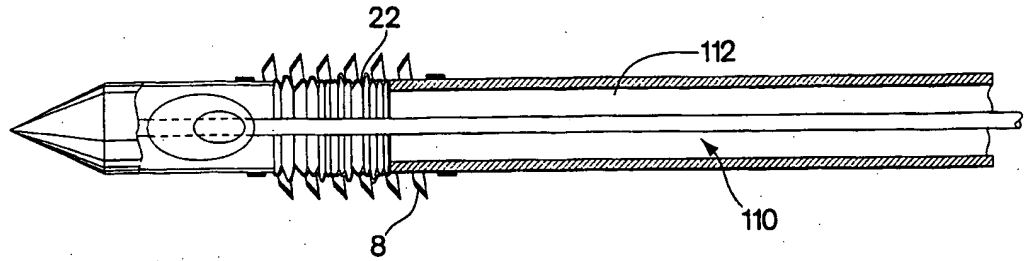


Fig. 9A

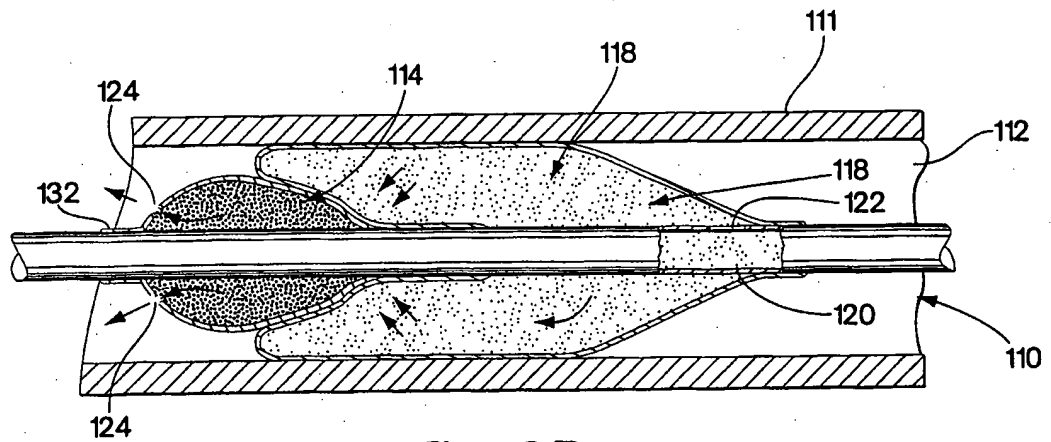


Fig. 9B

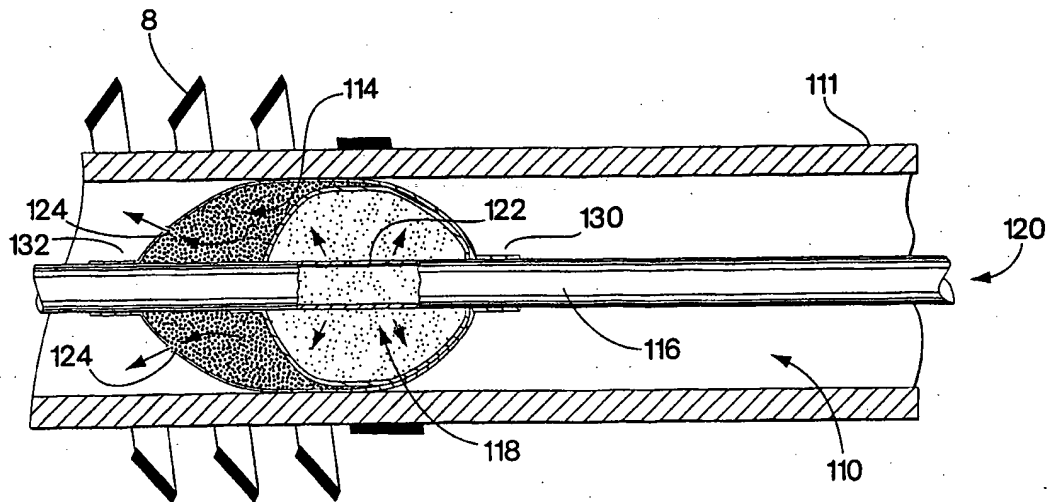


Fig. 9C



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : A61F 2/06	A3	(11) International Publication Number: WO 00/18302 (43) International Publication Date: 6 April 2000 (06.04.00)
(21) International Application Number: PCT/US99/22553 (22) International Filing Date: 30 September 1999 (30.09.99) (30) Priority Data: 09/163,884 30 September 1998 (30.09.98) US (71) Applicant: C. R. BARD, INC. [US/US]; 730 Central Avenue, Murray Hill, NJ 07974 (US). (72) Inventors: GAMBALE, Richard, A.; 382 Dunstable Road, Tyngsboro, MA 01879 (US). AHERN, John, E.; 30 Lynn Fells Parkway, Melrose, MA 02176 (US). PARASCAN- DOLA, Michael; 14 Hazelnut Lane, Londonderry, NH 03053 (US). (74) Agent: PERULLO, John, F.; Kirkpatrick & Lockhart LLP, 75 State Street, Boston, MA 02109-1808 (US).		(81) Designated States: CA, JP, MX, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). Published <i>With international search report.</i> (88) Date of publication of the international search report: 21 September 2000 (21.09.00)
(54) Title: IMPLANT DELIVERY SYSTEM (57) Abstract <p>The present invention provides an implant delivery system for placing interior defining implants in the human body. The devices comprise elongate shafts and a mechanism at the distal end of the shaft for engaging and retaining the implant in place on the shaft during delivery through the vessels and insertion of the distal end of the shaft into tissue. One embodiment employs a flexible outer tube at its distal end that compresses and crinkles to a larger diameter upon being compressed lengthwise to engage the inside surface of the implant. Another embodiment utilizes a tubular delivery shaft having a cross section with segments of oval shaped cross sections which serve to engage the inside of implant located on the shaft. A cam slidable within the shaft engages the oval areas, deforming them to a circular shape which permits the implants to be released.</p> <div data-bbox="909 1134 1315 1764" data-label="Image"> </div>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon	KR	Republic of Korea	PL	Poland		
CN	China	KZ	Kazakhstan	PT	Portugal		
CU	Cuba	LC	Saint Lucia	RO	Romania		
CZ	Czech Republic	LI	Liechtenstein	RU	Russian Federation		
DE	Germany	LK	Sri Lanka	SD	Sudan		
DK	Denmark	LR	Liberia	SE	Sweden		
EE	Estonia			SG	Singapore		

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US 99/22553

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 5, 9, 13, 17, 21
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:
1-4, 6-8

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 99/22553

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61F2/06

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 690 643 A (WIJAY BANDULA) 25 November 1997 (1997-11-25) abstract; figures 1,2 ---	1,2,6-8
X	EP 0 717 969 A (TARGET THERAPEUTICS INC) 26 June 1996 (1996-06-26) column 9, line 26 - line 45; figures 4-6 ---	1,2
X	US 5 755 682 A (GIESE WILLIAM L ET AL) 26 May 1998 (1998-05-26) column 23, line 53 - line 67; figures 11A-11C ---	1,2
A	US 5 810 836 A (HUSSEIN HANY ET AL) 22 September 1998 (1998-09-22) cited in the application abstract; figures 7-10 -----	1-4,6-8

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

* & * document member of the same patent family

Date of the actual completion of the international search

16 February 2000

Date of mailing of the international search report

- 6. JULI 2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Hansen, S

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US 99/22553

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 5, 9, 13, 17, 21
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:
1-4, 6-8

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
☐ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

1. Claims: 1-4,6-8

A delivery device for an hollow implant comprising:
an elongated shaft having proximal and distal ends and a lumen;
at least one deformable surface adjacent to the distal end that can be deformed to contact an inside surface of an implant and reformed to release the implant.

2. Claims: 10-12

An implant delivery device comprising:
a tubular shaft having a lumen and proximal and distal ends;
a plunger having a proximal side and a distal side configured to hold an implant and the plunger being slidable and fluid tight engagement with the lumen at the distal end of the shaft such that pressurization of fluid contained within the lumen causes the plunger to move in a distal direction.

3. Claims: 14-16

An implant delivery device comprising:
an outer delivery shaft having a lumen;
an inner shaft having a lumen;
a first bladder with perfusion ports sealed around the shaft, defining an interior with a volumen and containing a therapeutic substance within the interior and; a second bladder sealed around the shaft in close proximity to the first bladder and in fluid communication with the lumen.

4. Claims: 18-20

A delivery system for implanting a device in tissue in a patient comprising:
a shaft having proximal and distal ends and means for temporarily restraining an implant at the distal end;
a depth monitor mechanism having a sensor at the distal end of the shaft and indicator means joined to the proximal end of the shaft.

5. Claims: 22,23

An implant delivery system for placing a device in a patient comprising:
a shaft having proximal and distal ends;
a mechanism for releasably retaining an implant at the distal end of the shaft;
a navigation system having components internal and external to the patient including sensors mounted on the shaft.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/JS 99/22553

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5690643 A	25-11-1997	WO 9729720 A	21-08-1997
EP 0717969 A	26-06-1996	US 5814062 A	29-09-1998
		AU 4056095 A	27-06-1996
		CA 2165597 A	23-06-1996
		JP 8238320 A	17-09-1996
US 5755682 A	26-05-1998	AU 716771 B	09-03-2000
		AU 4057397 A	06-03-1998
		DE 19735141 A	30-04-1998
		EP 0959815 A	01-12-1999
		GB 2316322 A,B	25-02-1998
		JP 2886847 B	26-04-1999
		JP 10146350 A	02-06-1998
		NO 990688 A	12-04-1999
		WO 9806356 A	19-02-1998
		US 5944019 A	31-08-1999
US 5810836 A	22-09-1998	EP 0891172 A	20-01-1999
		WO 9732551 A	12-09-1997
		US 5971993 A	26-10-1999
		US 6053924 A	25-04-2000
		US 5878751 A	09-03-1999

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☒ FADED TEXT OR DRAWING
- ☒ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.